

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

JUN 18 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130570</u>	
Name	<u>C. RITALA</u>	ID#	<u>3791</u> Date <u>6/14/10</u>
Agency	<u>APD</u>	Phone #	<u>786-2640</u>
Instrument Location	<u>FLORA SUB (4th Ave)</u>		
Alco S/N <u>X301600</u>		Target Value <u>.084</u>	High Pressure <u>500</u>
Alco Test Values <u>.082</u>		<u>.082</u>	
1 st Alco		2 nd Alco	
Signature <u>[Signature]</u>		<u>Ritala/1349</u>	<u>003</u> <u>6/21/10</u>
(OVER)			

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 21st day of July, 2010.

[Signature]
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N


130570 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

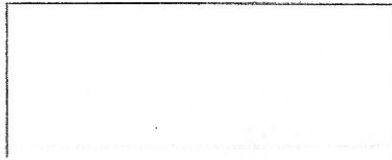

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130570 ✓

JUNE 14, 2010 ✓

OPERATOR'S NAME:

RITALA

OPERATOR'S NUMBER: 3791

SUBJECT'S LAST NAME:

VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI :

SIXTY DAY

O.L. #: A

DEPT/AGENCY: ANCI

CASE/REPORT: A

TEST TYPE: V

ALCO TARGET VALUE: .084 ✓


ALCO S/N: X301600 ✓

--- BREATH ANALYSIS ---

.084 ADJUSTED FOR 30.20 in ✓
ALCO TARGET .084 17:59
BLANK TEST .000 18:00
INTERNAL STANDARD VERIFIED 18:00
ALCO TV 30.20 in .082 ✓ 18:00
BLANK TEST .000 ✓ 18:01
SUBJECT SAMPLE .000 18:02
BLANK TEST .000 ✓ 18:02
ALCO TV 30.20 in .082 ✓ 18:03
BLANK TEST .000 18:03



DIAGNOSTIC CHECK

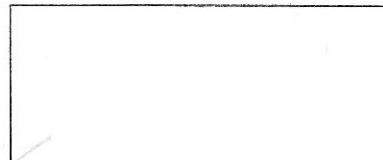

ALASKA DEPARTMENT OF PUBLIC SAFETY
ATAMASTER cdm 130570 ✓

JUNE 14, 2010 ✓

TIME 17:57

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 12/11/08
HEATERS
SAMPLE CHAMBER: 50c
BREATH TUBE: 41c
BAROMETER: 30.20 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST
!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGH
IJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnopqrstuvwxyz{|}~`

